


# ERGOMETER PLACEMENT FOR INDOOR ACTIVITY

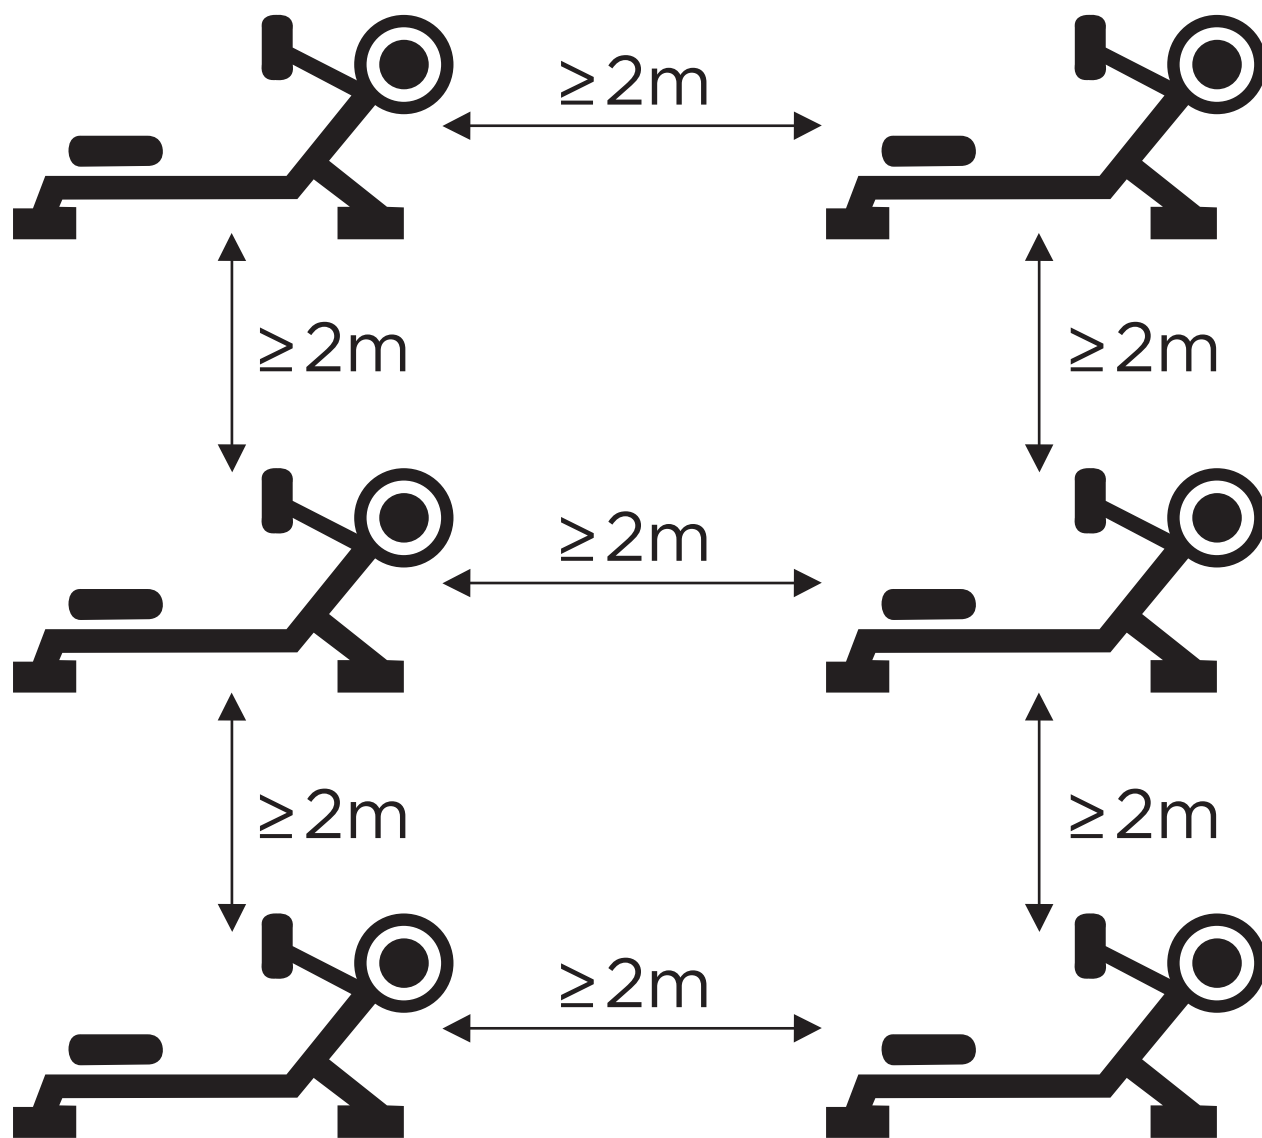

Ergometers must be spaced with at least 2m between each in all directions. The 2m should be measured “elbow to elbow” when side-by-side and from the front of an ergometer to maximal “lay back” of the ergometer immediately in front.